

Usual and Advanced Monitoring in Patients Receiving Oxygen Therapy

François Lellouche and Erwan L'Her

Introduction

Usual Monitoring of Patients on Oxygen Therapy

Clinical Evaluation

Breathing Frequency

Pulse Oximetry

Oxygen Requirements (F_{IO_2} or Oxygen Flow)

Minute Ventilation

Arterial Blood Gas Analysis

Advanced Monitoring for Patients on Oxygen Therapy

Early Warning Scores

New Automated and Continuous Scoring Systems Derived From Wearable Sensors

New Automated and Continuous Scoring Systems Derived From Automated Oxygen Titration

Summary

Respiratory monitoring in patients receiving oxygen therapy for acute care is mandatory at the initial stage of in-hospital management given the potential risk of clinical worsening. Although some patients benefit from close monitoring in the ICU, the vast majority of them are managed in general wards with reduced staff and clinical supervision. The objective of monitoring is to detect early clinical deterioration, which may help prevent in-hospital cardiac arrest. In addition to the clinical and usual evaluations (eg, breathing frequency, breathing pattern, oximetry, and oxygen flow requirements), early warning scoring systems have been developed to detect clinical deterioration in acutely ill patients. The monitoring of these scores is recommended for patients receiving oxygen therapy. These scores have several limitations, among which is the absence of oxygen flow evaluation. Manual and intermittent monitoring of these scores in the ward is time-consuming and may not be sufficient to accurately detect deterioration of patient's clinical condition in a timely manner. Automated and continuous monitoring, in addition to clinical evaluation and arterial blood gases analysis, which remain necessary, may improve the detection of clinical worsening in specific patients. Devices that automatically titrate and wean oxygen flow on the basis of S_{pO_2} enable measurement of several major cardiorespiratory parameters (eg, S_{pO_2} , oxygen flow, heart rate, breathing frequency, and heart rate variability). The combination of these parameters into new scores is at least as accurate and well-evaluated, and recommended early warning scores and may be useful in monitoring patients receiving oxygen therapy. *Key words:* acute respiratory failure; COPD; oxygen therapy; respiratory monitoring; oximetry; oxygen flow; breathing frequency; early warning scores; automated oxygen therapy. [Respir Care 0;0(0):1–●. © 0 Daedalus Enterprises]

OXYGEN THERAPY MONITORING

Introduction

In-hospital cardiac arrest remains a frequent event, with almost 300,000 occurring every year among adult patients in the United States.¹ This is nearly 10 times higher than the annual motor vehicle fatality rate in United States.² Cardiac arrest is most frequently due to cardiac causes (50–60%) or respiratory insufficiency (15–40%). Contrary to out-of-hospital cardiac arrests, in-hospital cardiac arrests are considered preventable because hospitalized patients, usually managed during the acute phase of their illness, are closely monitored.³ In most cases, a deterioration of the clinical condition occurs prior to an in-hospital cardiac arrest.⁴ Prevention is therefore recommended with early identification of at-risk patients combined with early interventions, such as rapid response teams.⁵ The first step is the identification of clinical condition worsening with the usual monitoring tools (eg, vital signs, biological signs) and with scoring systems based on multiple criteria. Many scoring systems have been developed based on the concept of an early warning scoring (EWS) system, published > 20 years ago.⁶ These scores, however, are difficult to implement, and results of these scoring systems are not generalizable across heterogeneous hospitals systems.^{7,8} It is likely that many patients receive oxygen therapy before cardiac arrest, especially if cardiac arrest is related to respiratory insufficiency. Surprisingly, oxygen flow is not part of the EWS systems, even though this is a major parameter used by clinicians to evaluate the severity of a patient's illness. This discrepancy will be discussed in this review. In patients receiving oxygen therapy, clinical evaluation and close monitoring are essential, including breathing frequency, signs of respiratory distress, and other physiological parameters related to oxygen needs.⁹ In addition, the close monitoring of physiological parameters is recommended for patients receiving conventional oxygen therapy, and S_{pO_2} should be used "in all breathless and acutely ill patients."¹⁰ The British Thoracic Society also recommends the use of a physiological track and trigger system such as the National

Early Warning Score (NEWS) to monitor patients receiving oxygen therapy.^{10,11}

We review several monitoring parameters and scoring systems recommended for patients receiving oxygen therapy and discuss the limitations of current scores. We will then present a new score, the Early Warning Score_{O₂}, which is dedicated to patients receiving oxygen therapy, and includes the oxygen flow. This score was designed in the context of the development of automated oxygen titration devices.

Usual Monitoring of Patients on Oxygen Therapy

Clinical Evaluation

Clinical evaluation is required to evaluate the severity of illness in patients receiving oxygen therapy, and visually monitoring a patient may provide more information on the patient's condition than any scores. In addition to the basic vital signs (eg, pulse, breathing frequency, arterial pressure, temperature), the breathing pattern, signs of hemodynamic shock, and encephalopathy must be evaluated in acutely ill patients to detect signs of low peripheral perfusion and signs of respiratory distress (Fig. 1).¹² Other essential parameters to evaluate patients receiving oxygen therapy include breathing frequency, oxygenation parameters (S_{pO_2} and oxygen supplementation requirements), and arterial blood gases. However, such monitoring, which implies repeated evaluations of several parameters, is time-consuming and not frequently performed due to staff overload, and thus it may not be sufficient to detect a patient's deterioration, especially in units with reduced monitoring (eg, outside ICUs) where continuous monitoring of clinical and physiological parameters is not feasible.¹³

Breathing Frequency

Clinical events before in-hospital cardiac arrest are typically respiratory events with increased breathing frequency.¹⁴ Breathing frequency is among the first vital signs to change in deteriorating patients, and it has been reported to be the best individual predictor of cardiac arrest in general wards.⁹ However, the usual vital parameters, including S_{pO_2} values and breathing frequency, are insufficiently monitored in patients in the general ward before severe outcomes such as cardiac arrest, ICU admission, or unexpected death.^{3,15} This parameter is well correlated with other signs of respiratory distress.¹⁶ The current method to evaluate breathing frequency in spontaneously breathing patients outside ICU is the visual measurement of breathing in a given time. Measurement of breathing frequency is commonly performed by manually counting the chest movements of the individual over a period of 15–60 s.¹⁷ This practice is time-consuming and prone to

Dr Lellouche is affiliated with Centre de Recherche de l'Institut Universitaire de Cardiologie et de Pneumologie de Québec, Québec, Québec, Canada. Dr L'Her is affiliated with CHU La Cavale Blanche, Brest, France.

Drs Lellouche and L'Her are co-founders, shareholders, and directors of Oxynov, a research and development company that designed and marketed the automated oxygen adjustment system (FreeO₂) used in this work.

Correspondence: François Lellouche MD PhD, Centre de Recherche de l'Institut Universitaire de Cardiologie et de Pneumologie de Québec, 2725 Chemin Sainte-Foy, G1V4G5, Québec, QC, Canada. E-mail: francois.lellouche@criucpq.ulaval.ca.

DOI: 10.4187/respcare.07623

OXYGEN THERAPY MONITORING

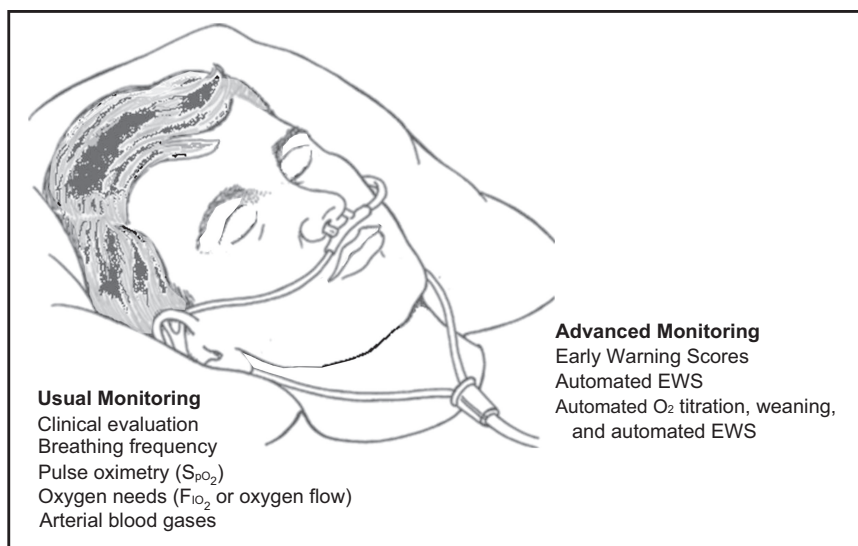


Fig. 1. Usual and advanced monitoring for acutely ill patients receiving oxygen therapy. EWS = Early Warning Scoring.

large variation in estimates of breathing frequency. Typically, the number of breaths occurring within 15 s is counted and then multiplied by 4 to give an estimate of breaths/min, which is therefore quantized into units of 4 breaths/min. This cumbersome method has to be repeated by nurses or other clinicians several times a day and is prone to operator variability. In daily practice, this parameter may not be adequately recorded.¹⁸

Recently, L'Her et al¹⁹ demonstrated that breathing frequency could be obtained from photoplethysmography tracings. The breathing frequency derived from pulse oximetry signals correlated very well with breathing frequency measured manually, even in subjects with atrial fibrillation.¹⁹ This function has been incorporated into some automated oxygen titration and weaning systems, enabling the continuous measurement of breathing frequency in patients wearing a pulse oximetry device.¹⁹

Pulse Oximetry

Pulse oximetry is usually considered accurate to evaluate and monitor blood oxygenation²⁰ and is considered the fifth vital sign.^{10,20} Differences may exist between oximetry devices, although it is usually considered that several oximeters from different leading companies are equivalent in terms of accuracy for S_{pO_2} values $> 80\%$ when tested in optimal conditions with healthy subjects.²¹⁻²³ However, differences between oximeters tend to be more pronounced when the comparisons are conducted in patients.²⁴⁻²⁷

Oximetry measurements have well-known limitations, such as dyshemoglobinemia, polished fingernails, darkly pigmented skin, low perfusion, and motion artefact.^{20,28} Oximetry inaccuracies are frequently reported in the case of low S_{pO_2} (ie, $< 80\%$) and in the case of darkly pigmented

skin.^{21,22} However, several technical improvements have increased the accuracy of the signal in difficult situations. Jubran and Tobin²⁹ reported in 1990 that $S_{pO_2} > 95\%$ was required to obtain sufficient oxygenation in populations with darkly pigmented skin. Currently, the differences among oximetry devices are negligible for usual levels of S_{pO_2} . During severe hypoxemia, however, a gap of a few mm Hg still exists between S_{aO_2} and S_{pO_2} . In several studies by one group, oximeters overestimated S_{pO_2} by 2.5–5 mm Hg in comparison with S_{aO_2} in subjects with darkly pigmented skin, especially at very low values (ie, $< 70\%$) and with large standard deviations.^{21,22,24} Among well-recognized pulse oximeters (eg, Masimo, Nonin, and Nellcor), the bias with reference values (ie, S_{aO_2}) were low whatever the color skin when S_{aO_2} or S_{pO_2} values were $> 80\%$.²² In the same study, bias of $\pm 4\%$ still existed with very low S_{pO_2} values (ie, 60–70%), and differences up to 10% could be detected in S_{pO_2} values among the tested devices during severe hypoxemia, especially when disposable sensors were used.²² Yamamoto et al³⁰ reported that polished fingernails had only minor impact on S_{pO_2} measurements. In another study conducted in 33 healthy women, several polish colors were tested and the authors noted moderately reduced S_{pO_2} values with specific colors (ie, blue, beige, purple, and white), but the tested oximeters were not among the reference oximeters.³¹

Monitoring of pulse oximetry alone did not demonstrate an impact on patient outcomes.³² This may be explained by liberal oxygen administration, which is largely used to avoid hypoxemia. In addition, in a health care system with few hypoxemia events, S_{pO_2} is not a good marker of severity, and the level of oxygen flow should instead be used to evaluate respiratory severity. Interestingly, intermittent pulse oximetry monitoring has been reported to be

OXYGEN THERAPY MONITORING

inaccurate to detect episodes of hypoxemia after general surgery.³³ In > 800 subjects after noncardiac surgeries, continuous S_{pO_2} monitoring was performed with blinded results for clinicians. Hypoxemia was frequent, but 90% of the episodes were missed by nurses with intermittent S_{pO_2} measurements.³³

Oxygen Requirements (F_{IO_2} or Oxygen Flow)

How many times have we explained to students that S_{pO_2} or P_{aO_2} provided alone, without mentioning the oxygen requirements (in L/min or as F_{IO_2}) is useless to assess a patient's illness severity? For patients receiving mechanical ventilation, ARDS severity is categorized based on P_{aO_2}/F_{IO_2} ³⁴ or S_{pO_2}/F_{IO_2} .³⁵ In nonintubated patients, S_{pO_2} or P_{aO_2} should be interpreted while considering F_{IO_2} (or estimated F_{IO_2} ³⁶) to evaluate a patient's illness severity. Surprisingly, there is no EWS that incorporates oxygen flow or F_{IO_2} , although many incorporate S_{pO_2} .³⁷ Some EWS systems incorporate oxygen requirements, but only in a binary fashion that evaluates if oxygen supplementation is used.³⁷ To our knowledge, only one score derived from NEWS incorporated a semiquantitative evaluation of oxygen flow, even though a patient with an oxygen flow of 2 L/min or 10 L/min (equivalent to 0.30 or 0.60 F_{IO_2} ³⁶) are not equivalent!³⁸

In comparison with several preexisting models (ie, EWS, Modified EWS [MEWS], and VitalPac EWS [ViEWS]), the S_{pO_2}/F_{IO_2} ratio showed comparable or better predictive accuracy for unexpected ICU transfers in the respiratory wards and for mortality prediction.³⁹ The F_{IO_2} , in addition to breathing frequency and S_{pO_2} , was also used to predict outcome with high-flow nasal cannula therapy.⁴⁰

With automated oxygen titration devices, the oxygenation parameters (S_{pO_2} and oxygen flow or corresponding equivalent F_{IO_2}) and respiratory parameters are continuously monitored, and respiratory scores that include these parameters and trends may be helpful in monitoring patients receiving oxygen therapy (see below).

Minute Ventilation

Minute ventilation is a relevant and desirable parameter of monitoring for patients with respiratory failure or for patients receiving sedation.⁴¹ In patients who are not on invasive or noninvasive mechanical ventilation, however, this parameter may be difficult to accurately measure in daily practice. Respiratory inductive plethysmography has been used for research purposes to measure tidal volume, breathing frequency, but it requires multiple calibrations and is not adapted for typical care.⁴² A bio-impedance respiratory volume monitor (ExSpirom, Respiratory Motion, Waltham, Massachusetts) has been proposed and tested during procedural sedations, and it has produced interesting results in detecting apnea or hypoventilation in

postoperative care.⁴³⁻⁴⁵ However, this monitoring is not recommended in the daily practice for patients receiving oxygen therapy for respiratory failure.¹⁰

Arterial Blood Gas Analysis

In patients with potential increased P_{aCO_2} (ie, patients with suspected or known CO_2 retention and especially in the case of loss of consciousness) and in patients with suspected metabolic disorders (eg, renal insufficiency, shock states, or specific intoxications), arterial blood gas analysis with lactate dosage may be required at the initiation of management and then as needed based on the patient's clinical evolution.¹⁰ Arterial blood gas analysis is mainly used to measure pH, P_{aCO_2} , and bicarbonates. P_{aO_2} values are not required when S_{pO_2} can be measured, especially if oxygenation recommendations are followed (ie, if S_{pO_2} is maintained at 88–92% or 90–94%). The prescription of long-term oxygen therapy may be an exception, and P_{aO_2} may be then required to decide on the initiation of this treatment.⁴⁶ In other situations, capillary blood gas analysis may be sufficient for the clinician's decision-making and preferred for the patient's comfort.⁴⁷ A meta-analysis of the studies comparing arterial and capillary blood gas measurements, pH, P_{aCO_2} , and bicarbonates values were well correlated.⁴⁸ Several noninvasive measurements of CO_2 may be alternatives to arterial blood gas analysis for CO_2 monitoring, such as capnography (end-tidal CO_2 measurements) and transcutaneous CO_2 measurements. In mechanically ventilated patients, capnography has been evaluated extensively, although in extubated patients the data are not convincing during procedural sedations or in patients with respiratory failure.^{49,50} Similarly, transcutaneous arterial CO_2 measurements have shown mixed results and cannot replace arterial blood gas analysis.⁵¹⁻⁵⁴

Advanced Monitoring for Patients on Oxygen Therapy**Early Warning Scores**

The concept of the EWS was developed over; 20 years ago.⁶ The scoring system has been developed for the early recognition of patients at risk for clinical deterioration.⁵⁵ In-hospital patients managed for acute respiratory failure are frequently on oxygen therapy, and many are at risk of early deterioration. Data indicate that 10–20% of the patients managed for community-acquired pneumonia requiring hospitalization will be transferred to an ICU,^{56,57} and the same proportion require ICU admission within 72 h. Carr et al⁵⁸ evaluated a registry of cardiopulmonary arrest events that occurred within 72 h of hospital admission; 12% occurred in patients with preexisting pneumonia, and among those patients with pneumonia, almost 40% of

OXYGEN THERAPY MONITORING

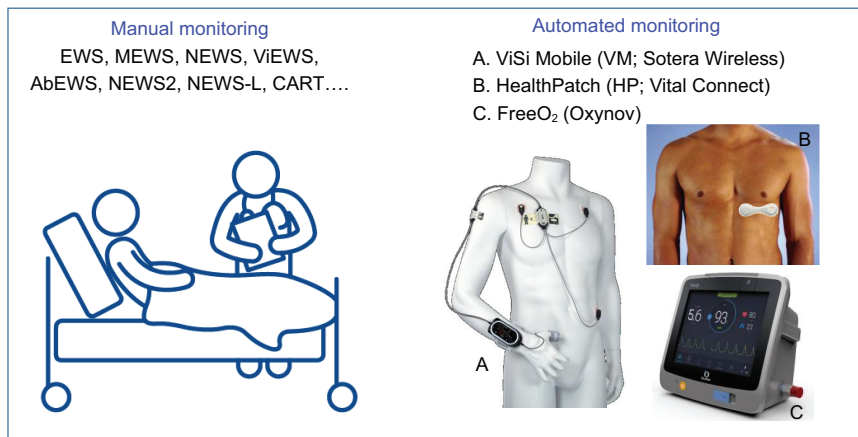


Fig. 2. Advanced monitoring with manual and automated recording of Early Warning Scoring (EWS) systems. MEWS = modified EWS; NEWS = National EWS, ViEWS = VitalPac EWS; AbEWS = abbreviated VitalPac; NEWS2 = National EWS 2; NEWS-L = NEWS-lactate; CART = Cardiac Arrest Risk Triage.

cardiac arrests occurred outside the ICU setting.⁵⁸ Viral pneumonia may have an even worse outcome,⁵⁹ and approximately 30% of patients managed for COVID-19 required management in the ICU.^{60,61}

Many scores have been developed to monitor in-hospital patients: EWS, MEWS, NEWS, ViEWS, Abbreviated VitalPac (AbEWS), NEWS2, Hamilton EWS (HEWS), Nottingham University EWS (NUH-EWS), Chronic Respiratory EWS (CREWS), NEWS-Lactate, Cardiac Arrest Risk Triage (CART), among others.⁶²⁻⁶⁸ There are > 100 different published track-and-trigger systems, most of which have been modified from the original EWS and developed using expert opinion, which has demonstrated variable levels of reliability, validity, and usefulness.^{69,70} Meta-analyses have been conducted to evaluate the impact of the implementation of these scores on outcomes⁵⁵ NEWS, which combines physiological parameters such as breathing frequency, S_{pO_2} , delivery of oxygen (or not), pulse rate, systolic blood pressure, level of consciousness, and temperature, may be beneficial for predicting patient deterioration.⁶⁵ However, a general conclusion cannot be generated due to heterogeneity in the way the score is used in studies and in populations studied.⁷ Monitoring any EWS is recommended in hospitalized patients, especially when receiving oxygen.^{10,11} When compared to the Quick Sepsis-Related Organ Failure Assessment (qSOFA) and systemic inflammatory response syndrome (SIRS), NEWS was found to be the most accurate for the detection of all sepsis end points.^{71,72} The introduction of the NEWS score did not change patient outcomes in several recent evaluations, although the NEWS score can predict outcome and determine the patient's illness severity when evaluated at the emergency department and after admission.⁷³⁻⁷⁵ One of several issues regarding these scoring systems is that the recording of all parameters is time-consuming and frequently

incomplete.¹⁵ In addition, these scores provide only an intermittent view of a patient's condition, and deterioration between 2 evaluations may be missed.⁷⁶

Results of a study by Hodgson et al⁷⁷ suggested that NEWS was less discriminative in predicting deterioration in subjects with respiratory disease compared to a population of unselected medical admissions. The NEWS2 score has been developed to take into account different S_{pO_2} targets in patients with COPD, but there is a debate on the utility of this new score in clinical practice.⁷⁸⁻⁸⁰

New Automated and Continuous Scoring Systems Derived From Wearable Sensors

New technologies have been developed to allow continuous monitoring in the medical setting with the aim to detect clinical deterioration earlier, to reduce work load, and to improve patient comfort (Fig. 2).⁸¹⁻⁸⁵ Several wireless and wearable sensors that allow continuous measurement of new scoring systems related to EWS have been evaluated in several studies, showing good accuracy and promising results for patient monitoring.^{76,86,87} In these studies, automated breathing frequency measurement was considered more accurate than measurements made by nurses. In addition, the detection of hypoxemia was more accurate with continuous measurements of S_{pO_2} than with intermittent measurements.³³

New Automated and Continuous Scoring Systems Derived From Automated Oxygen Titration

In patients receiving high-flow nasal cannula oxygen therapy, the ratio of pulse oximetry/ S_{pO_2} , defined as the ratio of S_{pO_2}/F_{IO_2} to breathing frequency (breaths/min), predicted the need for invasive mechanical ventilation.^{40,88}

OXYGEN THERAPY MONITORING

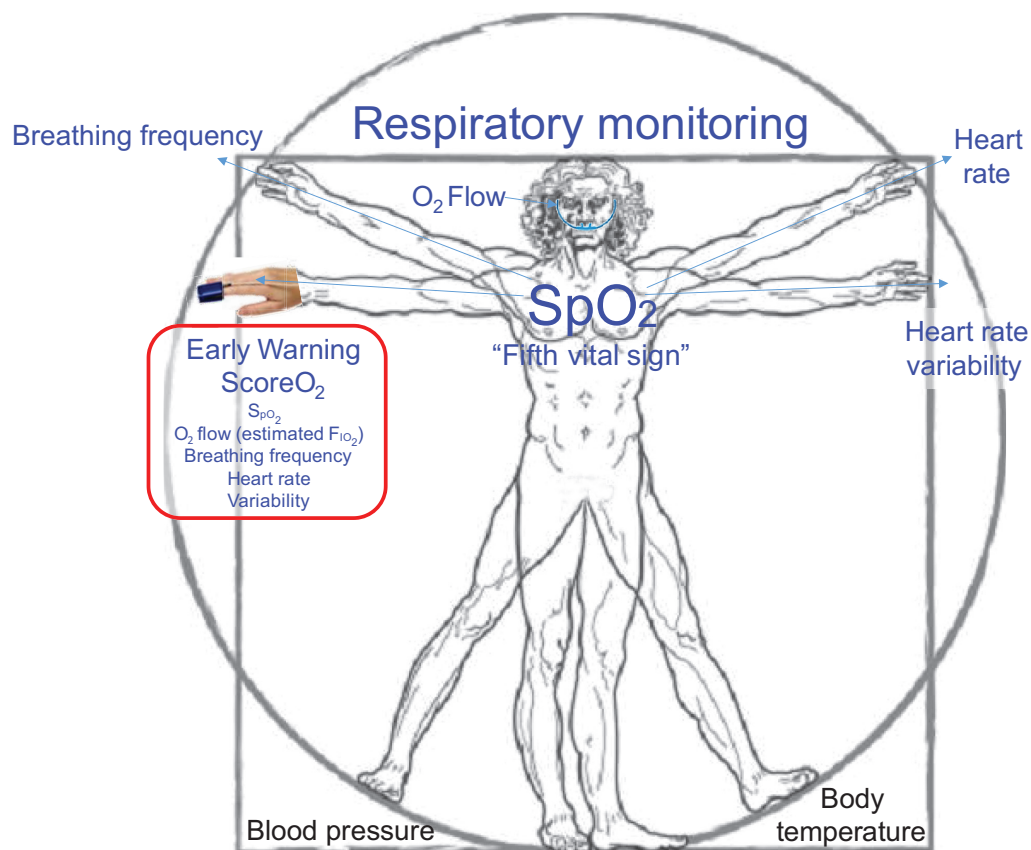


Fig. 3. Early Warning ScoreO₂ was developed from physiological parameters measured with the automated oxygen-titration device FreeO₂. O₂ flow (and estimated F_IO₂), S_pO₂, breathing frequency, and heart rate have been combined in this score. Variability is another parameter derived from photoplethysmography that can be used in the score.

This index cannot be transposed to conventional oxygen therapy, given the impact of nasal high-flow cannula therapy on breathing frequency.^{89,90} With automated oxygen titration (eg, with the FreeO₂ device, OxyNov, Quebec, Canada), which requires continuous pulse oximetry measurement, it is possible to continuously obtain several physiological values such as S_pO₂, oxygen flow, breathing frequency, heart rate, and heart rate variability. Indeed, in addition to the oxygen flow, which varies based on the patient's requirements to attain the S_pO₂ target, it is possible to obtain several important physiological parameters derived from the oximetry measurement.⁹¹ S_pO₂ and pulse rate are the main parameters obtained with pulse oximeters. Breathing frequency can be continuously measured with a specific algorithm based on photoplethysmographic signal analysis.¹⁹ Heart rate variability can also be measured with the photoplethysmographic signal analysis.¹⁹ With automated oxygen titration, it is possible to combine these measured parameters in a new EWS that is focused on patients on oxygen therapy (Early Warning ScoreO₂) (Fig. 3, Fig. 4). The Early Warning ScoreO₂, with several combinations of cardiorespiratory parameters provided by the

automated oxygen titration device, was at least as accurate as several well-validated scores (eg, NEWS, NEWS2, S_pO₂/F_IO₂) in 1,729 subjects in the emergency department setting and in 102 subjects in the ICU setting.^{92,93} Additional evaluations of these new scores are required to confirm the initial promising results. These automated and continuously measured scores may be useful for monitoring patients with acute respiratory failure on oxygen therapy, especially in the general ward. With the recent COVID-19 outbreak⁶¹ and other transmissible respiratory viruses (Middle East respiratory syndrome [MERS]⁹⁴, severe acute respiratory syndrome [SARS]⁹⁵), the need to reduce the interventions from health care workers at the patient's bedside to limit contaminations is an important goal. It may be achieved by automating the delivery and the monitoring of oxygen therapy, whereas almost all patients receive oxygen therapy when they require hospitalization.⁶¹

Summary

Respiratory monitoring is essential in patients receiving oxygen therapy for acute care, especially during the first

F3,F4

OXYGEN THERAPY MONITORING

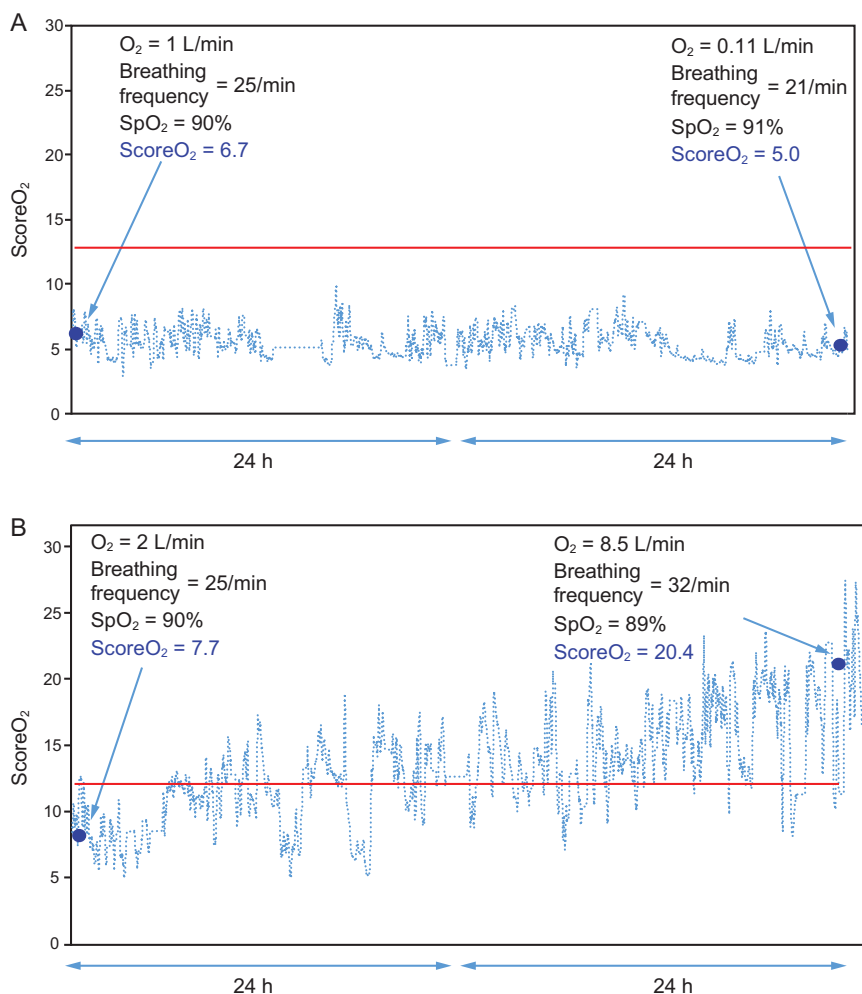


Fig. 4. Examples of variations of the Early Warning ScoreO₂ (ScoreO₂) during 48 h in 2 patients with COPD. A: One patient had a favorable clinical evolution; (B) the other patient had a poor clinical evolution. In both patients, the automated oxygen-titration device (FreeO₂) was set with a target S_{pO₂} of 90%. The patient with a favorable outcome had an initial breathing frequency of 35 breaths/min, received oxygen flow of 1.0 L/min, and had an Early Warning ScoreO₂ of 6.7. After 2 d, breathing frequency and oxygen flow decreased, and the resulting ScoreO₂ was 5.0. The patient with the poor outcome (ie, ICU admission and intubation) had an initial ScoreO₂ of 7.7 with a progressive increase to 20.4.

days after treatment initiation. A patient's clinical condition may rapidly improve, which should lead to a reduction of support, including oxygen therapy, and to the early detection of criteria for hospital discharge. A patient's clinical condition may also worsen rapidly to the point that more intensive monitoring, additional support, and potentially a reevaluation of treatment may be needed. Usual monitoring includes clinical oxygenation parameters and, for specific patients, arterial blood gas analysis. Advanced monitoring includes the utilization of EWS systems. The aim of EWS systems is to detect clinical worsening early. However, EWS systems have several limitations, including the lack of evaluation of oxygen requirements and manual and intermittent recording. Intermittent monitoring is a time-consuming and labor-intensive process, and it may miss

changes in a patient's clinical condition. This approach may not be optimal for the dynamic management of patients in a health care system under pressure with an increased number of fragile patients and a limited number of ICU beds. Automated and continuous monitoring may optimize patient care by improving the early detection of clinical deterioration while reducing the work load related to monitoring. Physiological parameters, including oxygen requirements, measured by devices that automatically deliver oxygen based on the S_{pO₂} have been combined. In initial evaluations, the new scores that stem from these simple parameters provide information that is at least as accurate as other EWS systems in detecting early deterioration of clinical conditions. These new scores may improve the monitoring of patients receiving oxygen therapy, but

OXYGEN THERAPY MONITORING

additional research is required to evaluate the impact on patient outcomes.

REFERENCES

- Andersen LW, Holmberg MJ, Berg KM, Donnino MW, Granfeldt A. In-hospital cardiac arrest: a review. *JAMA* 2019;321(12):1200-1210.
- National Highway Traffic Safety Administration. Motor vehicle fatality rate in U.S. by year. Available at: <https://www.nhtsa.gov/press-releases/early-estimates-traffic-fatalities-2019>. Accessed June 25, 2020.
- Galhotra S, DeVita MA, Simmons RL, Dew MA, Members of the Medical Emergency Response Improvement Team (MERIT) Committee. Mature rapid response system and potentially avoidable cardiopulmonary arrests in hospital. *Qual Saf Health Care* 2007;16(4):260-265.
- Andersen LW, Kim WY, Chase M, Berg KM, Mortensen SJ, Moskowitz A, et al. The prevalence and significance of abnormal vital signs prior to in-hospital cardiac arrest. *Resuscitation* 2016;98:112-117.
- Kronick SL, Kurz MC, Lin S, Edelson DP, Berg RA, Billi JE, et al. Part 4: systems of care and continuous quality improvement: 2015 American Heart Association guidelines update for cardiopulmonary resuscitation and emergency cardiovascular care. *Circulation* 2015;132(18 Suppl 2):S397-S413.
- Morgan R, Williams F, Wright M. An early warning scoring system for detecting developing critical illness. *Clin Intensive Care* 1997;8(2):100.
- Smith MEB, Chiovaro JC, O'Neil M, Kansagara D, Quiñones AR, Freeman M, et al. Early warning system scores for clinical deterioration in hospitalized patients: a systematic review. *Ann Am Thorac Soc* 2014;11(9):1454-1465.
- Maharaj R, Raffaele I, Wendon J. Rapid response systems: a systematic review and meta-analysis. *Crit Care* 2015;19(1):254.
- Churpek MM, Yuen TC, Huber MT, Park SY, Hall JB, Edelson DP. Predicting cardiac arrest on the wards: a nested case-control study. *Chest* 2012;141(5):1170-1176.
- O'Driscoll BR, Howard LS, Earis J, Mak V, BTS Emergency Oxygen Guideline Development Group. BTS guideline for oxygen use in adults in healthcare and emergency settings. *Thorax* 2017;72(Suppl 1):ii1-ii90.
- Centre for Clinical Practice at NICE (UK). Acutely Ill Patients in Hospital: Recognition of and Response to Acute Illness in Adults in Hospital. London: National Institute for Health and Clinical Excellence (UK); 2007.
- Vincent J-L. Definition, monitoring, and management of shock states. In: Gullo AL, Besso J, Williams GF, editors. *Intensive and critical care medicine*. Milan: Springer; 2009.
- Tobin MJ. Respiratory monitoring in the intensive care unit. *Am Rev Respir Dis* 1988;138(6):1625-1642.
- Schein RM, Hazday N, Pena M, Ruben BH, Sprung CL. Clinical antecedents to in-hospital cardiopulmonary arrest. *Chest* 1990;98(6):1388-1392.
- Ludikhuije J, Smorenburg SM, de Rooij SE, de Jonge E. Identification of deteriorating patients on general wards; measurement of vital parameters and potential effectiveness of the Modified Early Warning Score. *J Crit Care* 2012;27(4):424.e7-e13.
- Tulaimat A, Gueret RM, Wisniewski MF, Samuel J. Association between rating of respiratory distress and vital signs, severity of illness, intubation, and mortality in acutely ill subjects. *Respir Care* 2014;59(9):1338-1344.
- World Health Organization. Fourth Programme Report, 1988-1989: Acute Respiratory Infections Programme for Control of Acute Respiratory Infections. Geneva: World Health Organization; 1990.
- Cretikos MA, Bellomo R, Hillman K, Chen J, Finfer S, Flabouris A. Respiratory rate: the neglected vital sign. *Med J Aust* 2008;188(11):657-659.
- L'Her E, N'Guyen QT, Pateau V, Bodenes L, Lellouche F. Photoplethysmographic determination of the respiratory rate in acutely ill patients: validation of a new algorithm and implementation into a biomedical device. *Ann Intensive Care* 2019;9(1):11.
- Jubran A. Pulse oximetry. *Crit Care* 2015;19:272.
- Bickler PE, Feiner JR, Severinghaus JW. Effects of skin pigmentation on pulse oximeter accuracy at low saturation. *Anesthesiology* 2005;102(4):715-719.
- Feiner JR, Severinghaus JW, Bickler PE. Dark skin decreases the accuracy of pulse oximeters at low oxygen saturation: the effects of oximeter probe type and gender. *Anesth Analg* 2007;105(6 Suppl):S18-S23.
- Louie A, Feiner JR, Bickler PE, Rhodes L, Bernstein M, Lucero J. Four types of pulse oximeters accurately detect hypoxia during low perfusion and motion. *Anesthesiology* 2018;128(3):520-530.
- Foglia EE, Whyte RK, Chaudhary A, Mott A, Chen J, Probert KJ, Schmidt B. The effect of skin pigmentation on the accuracy of pulse oximetry in infants with hypoxemia. *J Pediatr* 2017;182:375-377.
- Richards NM, Giuliano KK, Jones PG. A prospective comparison of 3 new-generation pulse oximetry devices during ambulation after open heart surgery. *Respir Care* 2006;51(1):29-35.
- Ross PA, Newth CJ, Khemani RG. Accuracy of pulse oximetry in children. *Pediatrics* 2014;133(1):22-29.
- Singh AK, Sahi MS, Mahawar B, Rajpurohit S. Comparative evaluation of accuracy of pulse oximeters and factors affecting their performance in a tertiary intensive care unit. *J Clin Diagn Res* 2017;11(6):OC05-OC08.
- Sauty A, Uldry C, Debétaz LF, Leuenberger P, Fitting JW. Differences in PO₂ and PCO₂ between arterial and arterialized earlobe samples. *Eur Respir J* 1996;9(2):186-189.
- Jubran A, Tobin MJ. Reliability of pulse oximetry in titrating supplemental oxygen therapy in ventilator-dependent patients. *Chest* 1990;97(6):1420-1425.
- Yamamoto LG, Yamamoto JA, Yamamoto JB, Yamamoto BE, Yamamoto PP. Nail polish does not significantly affect pulse oximetry measurements in mildly hypoxic subjects. *Respir Care* 2008;53(11):1470-1474.
- Sütçü Çiçek H, Gümüş S, Deniz Ö, Yildiz S, Açıkel CH, Çakir E, et al. Effect of nail polish and henna on oxygen saturation determined by pulse oximetry in healthy young adult females. *Emerg Med J* 2011;28(9):783-785.
- Moller JT, Johannessen NW, Espersen K, Ravlo O, Pedersen BD, Jensen PF, et al. Randomized evaluation of pulse oximetry in 20,802 patients: II. Perioperative events and postoperative complications. *Anesthesiology* 1993;78(3):445-453.
- Sun Z, Sessler DI, Dalton JE, Devereaux PJ, Shahinyan A, Naylor AJ, et al. Postoperative hypoxemia is common and persistent: a prospective blinded observational study. *Anesth Analg* 2015;121(3):709-715.
- Force ADT, Ranieri VM, Rubenfeld GD, Thompson BT, Ferguson ND, Caldwell E, et al. Acute respiratory distress syndrome: the Berlin Definition. *JAMA* 2012;307(23):2526-2533.
- Rice TW, Wheeler AP, Bernard GR, Hayden DL, Schoenfeld DA, Ware LB. Comparison of the SpO₂/FIO₂ ratio and the PaO₂/FIO₂ ratio in patients with acute lung injury or ARDS. *Chest* 2007;132(2):410-417.
- Wettstein RB, Shelledy DC, Peters JI. Delivered oxygen concentrations using low-flow and high-flow nasal cannulas. *Respir Care* 2005;50(5):604-609.
- Smith GB, Prytherch DR, Schmidt PE, Featherstone PI. Review and performance evaluation of aggregate weighted 'track and trigger' systems. *Resuscitation* 2008;77(2):170-179.

OXYGEN THERAPY MONITORING

38. Forster S, Housley G, McKeever TM, Shaw DE. Investigating the discriminative value of Early Warning Scores in patients with respiratory disease using a retrospective cohort analysis of admissions to Nottingham University Hospitals Trust over a 2-year period. *BMJ Open* 2018;8(7):e020269.
39. Kwack WG, Lee DS, Min H, Choi YY, Yun M, Kim Y, et al. Evaluation of the SpO₂/FiO₂ ratio as a predictor of intensive care unit transfers in respiratory ward patients for whom the rapid response system has been activated. *PLoS One* 2018;13(7):e0201632.
40. Roca O, Caralt B, Messika J, Samper M, Szymf B, Hernández G, et al. An index combining respiratory rate and oxygenation to predict outcome of nasal high flow therapy. *Am J Respir Crit Care Med* 2019;199(11):1368-1376.
41. Lee LA, Caplan RA, Stephens LS, Posner KL, Terman GW, Voepel-Lewis T, et al. Postoperative opioid-induced respiratory depression: a closed claims analysis. *Anesthesiology* 2015;122(3):659-665.
42. Delorme M, Bouchard PA, Simon M, Simard S, Lellouche F. Effects of high-flow nasal cannula on the work of breathing in patients recovering from acute respiratory failure. *Crit Care Med* 2017;45(12):1981-1988.
43. Mathews DM, Oberding MJ, Simmons EL, O'Donnell SE, Abnet KR, MacDonald K. Improving patient safety during procedural sedation via respiratory volume monitoring: a randomized controlled trial. *J Clin Anesth* 2018;46:118-123.
44. Nichols RH, Blinn JA, Ho TM, McQuitty RA, Kinsky MP. Respiratory volume monitoring reduces hypoventilation and apnea in subjects undergoing procedural sedation. *Respir Care* 2018;63(4):448-454.
45. Sessler DI. Preventing respiratory depression. *Anesthesiology* 2015;122(3):484-485.
46. Long term domiciliary oxygen therapy in chronic hypoxic cor pulmonale complicating chronic bronchitis and emphysema. Report of the Medical Research Council Working Party. *Lancet* 1981;1(8222):681-686.
47. Dar K, Williams T, Aitken R, Woods KL, Fletcher S. Arterial versus capillary sampling for analysing blood gas pressures. *BMJ* 1995;310(6971):24-25.
48. Zavorsky GS, Cao J, Mayo NE, Gabbay R, Murias JM. Arterial versus capillary blood gases: a meta-analysis. *Respir Physiol Neurobiol* 2007;155(3):268-279.
49. van Loon K, van Rheineck Leyssius AT, van Zaane B, Denteneer M, Kalkman CJ. Capnography during deep sedation with propofol by nonanesthesiologists: a randomized controlled trial. *Anesth Analg* 2014;119(1):49-55.
50. Fujimoto S, Suzuki M, Sakamoto K, Ibusuki R, Tamura K, Shiozawa A, et al. Comparison of end-tidal, arterial, venous, and transcutaneous PCO₂. *Respir Care* 2019;64(10):1208-1214.
51. Rodriguez P, Lellouche F, Aboab J, Buisson CB, Brochard L. Transcutaneous arterial carbon dioxide pressure monitoring in critically ill adult patients. *Intensive Care Med* 2006;32(2):309-312.
52. Mummary V, Rogers E, Padmanaban V, Matthew D, Woodcock T, Bloch S. Transcutaneous carbon dioxide measurement is not a reliable alternative to arterial blood gas sampling in the acute medical setting. *Eur Respir J* 2019;53(4):1801726
53. Maniscalco M, Fuschillo S. A transcutaneous carbon dioxide monitor is a useful tool with known caveats. *Eur Respir J* 2019;54(4):1900918
54. Conway A, Tipton E, Liu WH, Conway Z, Soalheira K, Sutherland J, et al. Accuracy and precision of transcutaneous carbon dioxide monitoring: a systematic review and meta-analysis. *Thorax* 2019;74(2):157-163.
55. Alam N, Hobbelen EL, van Tienhoven AJ, van de Ven PM, Jansma EP, Nanayakkara PW. The impact of the use of the Early Warning Score (EWS) on patient outcomes: a systematic review. *Resuscitation* 2014;85(5):587-594.
56. Angus DC, Marrie TJ, Obrosky DS, Clermont G, Dremsizov TT, Coley C, et al. Severe community-acquired pneumonia: use of intensive care services and evaluation of American and British Thoracic Society Diagnostic criteria. *Am J Respir Crit Care Med* 2002;166(5):717-723.
57. Fine MJ, Auble TE, Yealy DM, Hanusa BH, Weissfeld LA, Singer DE, et al. A prediction rule to identify low-risk patients with community-acquired pneumonia. *N Engl J Med* 1997;336(4):243-250.
58. Carr GE, Yuen TC, McConville JF, Kress JP, VandenHoek TL, Hall JB, et al. Early cardiac arrest in patients hospitalized with pneumonia: a report from the American Heart Association's Get With The Guidelines-Resuscitation Program. *Chest* 2012;141(6):1528-1536.
59. Burk M, El-Kersh K, Saad M, Wiemken T, Ramirez J, Cavallazzi R. Viral infection in community-acquired pneumonia: a systematic review and meta-analysis. *Eur Respir Rev* 2016;25(140):178-188.
60. Huang C, Wang Y, Li X, Ren L, Zhao J, Hu Y, et al. Clinical features of patients infected with 2019 novel coronavirus in Wuhan, China. *Lancet* 2020 [Epub ahead of print] doi: CrossRef.
61. Wang D, Hu B, Hu C, Zhu F, Liu X, Zhang J, et al. Clinical characteristics of 138 hospitalized patients with 2019 novel coronavirus-infected pneumonia in Wuhan, China. *JAMA* 2020;323(11):1061.
62. Churpek MM, Yuen TC, Park SY, Meltzer DO, Hall JB, Edelson DP. Derivation of a cardiac arrest prediction model using ward vital signs. *Crit Care Med* 2012;40(7):2102-2108.
63. Jo S, Yoon J, Lee JB, Jin Y, Jeong T, Park B. Predictive value of the National Early Warning Score-Lactate for mortality and the need for critical care among general emergency department patients. *J Crit Care* 2016;36:60-68.
64. Jansen JO, Cuthbertson BH. Detecting critical illness outside the ICU: the role of track and trigger systems. *Curr Opin Crit Care* 2010;16(3):184-190.
65. Smith GB, Prytherch DR, Meredith P, Schmidt PE, Featherstone PI. The ability of the National Early Warning Score (NEWS) to discriminate patients at risk of early cardiac arrest, unanticipated intensive care unit admission, and death. *Resuscitation* 2013;84(4):465-470.
66. Prytherch DR, Smith GB, Schmidt PE, Featherstone PI. ViEWS: towards a national early warning score for detecting adult inpatient deterioration. *Resuscitation* 2010;81(8):932-937.
67. Fernando SM, Fox-Robichaud AE, Rochweg B, Cardinal P, Seely AJE, Perry JJ, et al. Prognostic accuracy of the Hamilton Early Warning Score (HEWS) and the National Early Warning Score 2 (NEWS2) among hospitalized patients assessed by a rapid response team. *Crit Care* 2019;23(1):60.
68. Eccles SR, Subbe C, Hancock D, Thomson N. CREWS: improving specificity whilst maintaining sensitivity of the National Early Warning Score in patients with chronic hypoxaemia. *Resuscitation* 2014;85(1):109-111.
69. Churpek MM, Adhikari R, Edelson DP. The value of vital sign trends for detecting clinical deterioration on the wards. *Resuscitation* 2016;102:1-5.
70. Gao H, McDonnell A, Harrison DA, Moore T, Adam S, Daly K, et al. Systematic review and evaluation of physiological track and trigger warning systems for identifying at-risk patients on the ward. *Intensive Care Med* 2007;33(4):667-679.
71. Churpek MM, Snyder A, Han X, Sokol S, Pettit N, Howell MD, et al. Quick sepsis-related organ failure assessment, systemic inflammatory response syndrome, and early warning scores for detecting clinical deterioration in infected patients outside the intensive care unit. *Am J Respir Crit Care Med* 2017;195(7):906-911.
72. Usman OA, Usman AA, Ward MA. Comparison of SIRS, qSOFA, and NEWS for the early identification of sepsis in the emergency department. *Am J Emerg Med* 2019;37(8):1490-1497.
73. Sutherasan Y, Theerawit P, Suporn A, Nongnuch A, Phanachet P, Kositchaiwat C. The impact of introducing the early warning scoring

OXYGEN THERAPY MONITORING

- system and protocol on clinical outcomes in tertiary referral university hospital. *Ther Clin Risk Manag* 2018;14:2089-2095.
74. McNeill G, Bryden D. Do either early warning systems or emergency response teams improve hospital patient survival? A systematic review. *Resuscitation* 2013;84(12):1652-1667.
 75. Kivipuro M, Tirkkonen J, Kontula T, Solin J, Kalliomäki J, Pauniahio SL, et al. National early warning score (NEWS) in a Finnish multidisciplinary emergency department and direct vs. late admission to intensive care. *Resuscitation* 2018;128:164-169.
 76. Weenk M, Koeneman M, van de Belt TH, Engelen L, van Goor H, Bredie S. Wireless and continuous monitoring of vital signs in patients at the general ward. *Resuscitation* 2019;136:47-53.
 77. Hodgson LE, Dimitrov BD, Congleton J, Venn R, Forni LG, Roderick PJ. A validation of the National Early Warning Score to predict outcome in patients with COPD exacerbation. *Thorax* 2017;72(1):23-30.
 78. Pimentel MAF, Redfern OC, Gerry S, Collins GS, Malycha J, Prytherch D, et al. A comparison of the ability of the National Early Warning Score and the National Early Warning Score 2 to identify patients at risk of in-hospital mortality: a multi-centre database study. *Resuscitation* 2019;134:147-156.
 79. Hodgson LE, Congleton J, Venn R, Forni LG, Roderick PJ. NEWS2: too little evidence to implement? *Clin Med (Lond)* 2018;18(5):371-373.
 80. O'Driscoll R, Bakerly N, Murphy P, Turkington P. NEWS2 needs to be tested in prospective trials involving patients with confirmed hypercapnia. *Resuscitation* 2019;139:369-370.
 81. Cardona-Morrell M, Prgomet M, Turner RM, Nicholson M, Hillman K. Effectiveness of continuous or intermittent vital signs monitoring in preventing adverse events on general wards: a systematic review and meta-analysis. *Int J Clin Pract* 2016;70(10):806-824.
 82. Watkins T, Whisman L, Booker P. Nursing assessment of continuous vital sign surveillance to improve patient safety on the medical/surgical unit. *J Clin Nurs* 2016;25(1-2):278-281.
 83. Boatman AA, Wylie BJ, Goldfarb I, Azevedo R, Pittel E, Ng C, Haberer JE. Wireless vital sign monitoring in pregnant women: a functionality and acceptability study. *Telemed J E Health* 2016;22(7):564-571.
 84. Sahandi R, Noroozi S, Roushan G, Heaslip V, Liu Y. Wireless technology in the evolution of patient monitoring on general hospital wards. *J Med Eng Technol* 2010;34(1):51-63.
 85. Zubiete ED, Luque LF, Rodríguez AV, González IG. Review of wireless sensors networks in health applications. *Conf Proc IEEE Eng Med Biol Soc* 2011;2011:1789-1793.
 86. Weenk M, van Goor H, Frietman B, Engelen LJ, van Laarhoven CJ, Smit J, et al. Continuous monitoring of vital signs using wearable devices on the general ward: pilot study. *JMIR Mhealth Uhealth* 2017;5(7):e91.
 87. Weenk M, van Goor H, van Acht M, Engelen LJ, van de Belt TH, Bredie S. A smart all-in-one device to measure vital signs in admitted patients. *PloS One* 2018;13(2):e0190138.
 88. Roca O, Messika J, Caralt B, Garcia-de-Acilu M, Sztrymf B, Ricard J-D, Masclans JR. Predicting success of high-flow nasal cannula in pneumonia patients with hypoxemic respiratory failure: the utility of the ROX index. *J Crit Care* 2016;35:200-205.
 89. Sztrymf B, Messika J, Bertrand F, Hurel D, Leon R, Dreyfuss D, et al. Beneficial effects of humidified high flow nasal oxygen in critical care patients: a prospective pilot study. *Intensive Care Med* 2011;37(11):1780-1786.
 90. Mauri T, Alban L, Turrini C, Cambiaghi B, Carlesso E, Taccone P, et al. Optimum support by high-flow nasal cannula in acute hypoxemic respiratory failure: effects of increasing flow rates. *Intensive Care Med* 2017;43(10):1453-1463.
 91. Hess DR. Pulse oximetry: beyond SpO₂. *Respir Care* 2016;61(12):1671-1680.
 92. Viglino D, L'her E, Maltais F, Maignan M, Lellouche F. Evaluation of a new respiratory monitoring tool "Early Warning Score O₂" for patients admitted at the emergency department with dyspnea. *Resuscitation* 2020;148:59-65.
 93. Lellouche F, Ferrière N, Bodenès L, Pateau V, Doulou J, L'Her E. NEWS, heart rate variability and Early Warning Score O₂ (EWS.O₂): predictors of poor outcomes in ICU patient under spontaneous ventilation? *American Journal of Respiratory and Critical Care Medicine* 2020;201:A1145.
 94. Arabi YM, Balkhy HH, Hayden FG, Bouchama A, Luke T, Baillie JK, et al. Middle East respiratory syndrome. *N Engl J Med* 2017;376(6):584-594.
 95. Yu IT, Li Y, Wong TW, Tam W, Chan AT, Lee JH, et al. Evidence of airborne transmission of the severe acute respiratory syndrome virus. *N Engl J Med* 2004;350(17):1731-1739.